



# 3-Axis Magnetometer on a Chip

**Philip Keller**

**MAGNETICS 2017**

*The International Forum on Magnetic Applications, Technologies & Materials*

JANUARY 18-19 • ORLANDO, FL

# Why magnetometers?

“You can only make as well as you can measure”

Joseph Whitworth  
1803-1887  
Engineer,  
entrepreneur,  
inventor,  
philanthropist




*Credit: Grace's Guide to British Industrial History*



# 3-Axis Hall Magnetometers

- Advantages:
  - All vector components
  - Any probe orientation
- Limitations:
  - Orthogonality
  - Sensor separation
  - Planar Hall Effect
  - Cost





*Credits:*

- LakeShore Cryotronics (Model 460)
- Magnetic Sciences Inc. (F.W. Bell 8030)
- Metrolab (THM7025)


# The first revolution

- Vertical Hall sensor
  - Integrated 3-axis sensors
- Advantages:
  - Simplified construction
  - ~100  $\mu\text{m}$  active volume
- Limitations:
  - Si: lower sensitivity, higher noise





# Additional advantages

- Integrated current source and amplifier
- Integrated temperature sensor
- “Spinning current” to minimize offset, Planar Hall Effect, and noise




Credit: presentation by D. Popovic (Senis) at IMMW-14




# The second revolution

- Integrated ADC
  - Digital interface
- Advantages:
  - Minimize system complexity & cost
  - Minimize errors from inductive voltages
  - Additional controls
  - Sensor arrays feasible
- Disadvantages:
  - ADC performance




# Architecture

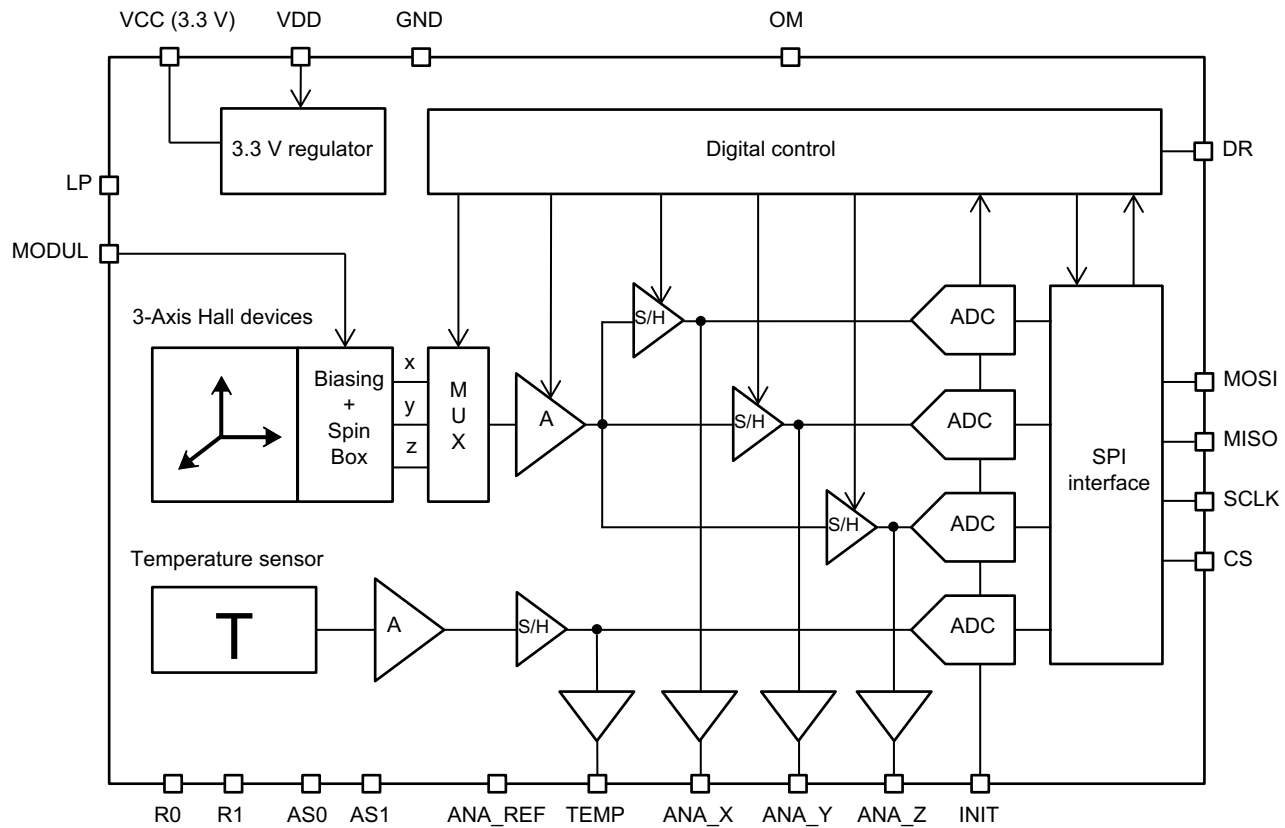

# Sensor arrays

- Communication:
  - SPI bus with individual Chip Select lines

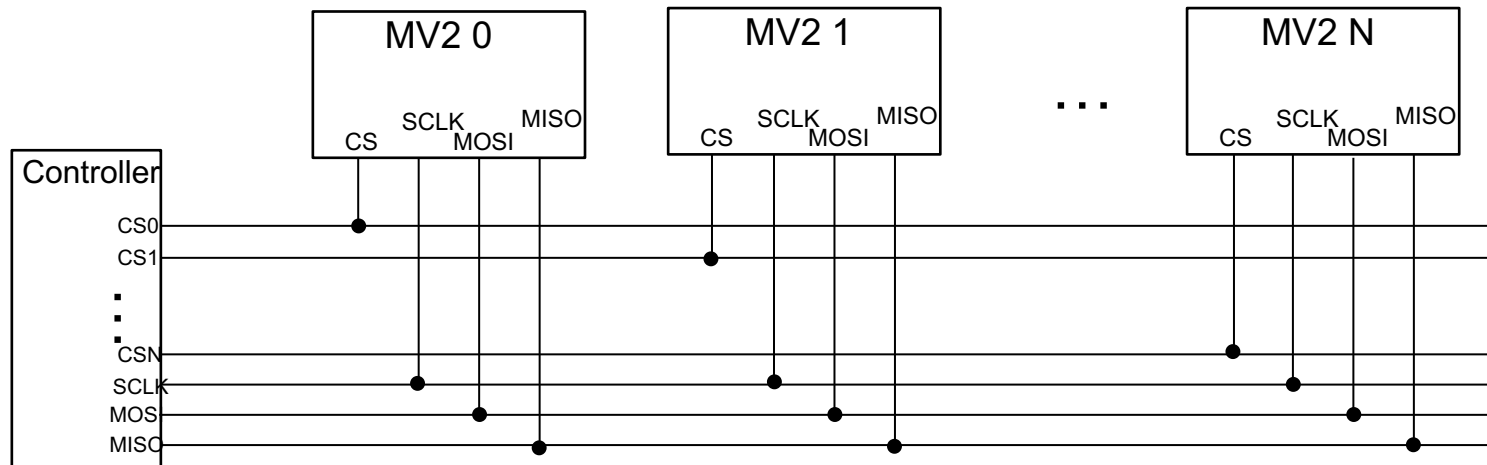


- Synchronization:
  - INIT 1 → 0: reinitialize and start ADC conversion



# Example: magnetron sputtering

- Magnets degraded by heat, radiation
- Causes uneven deposition
- Periodic mapping of magnets
- Sensor array:
  - Minimize downtime!
  - Simplify scanning robot




Credits:

- Wikipedia: "Sputter deposition"
- Dep. of Physics of Politecnico di Milano


# Example: Accelerator magnet mapping

- Facility for Antiproton and Ion Research (FAIR), Darmstadt, DE
- Dipoles of High-Energy Storage Ring (HESR)
- 44 bent dipoles, 4.2 m long, 0.17-1.7 T

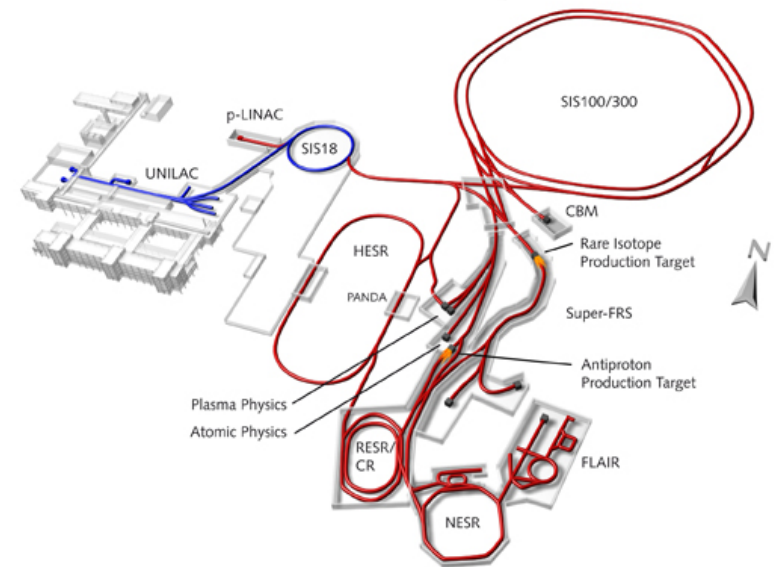


# Accelerator magnet mapper

- Angular map along entire magnet length
- 0.17, 0.5, 1.7 T
- $10^{-4}$  resolution
- 8 sensors
- Rotary motor for additional angles
- Sled for lengthwise motion
- 82 mm free gap

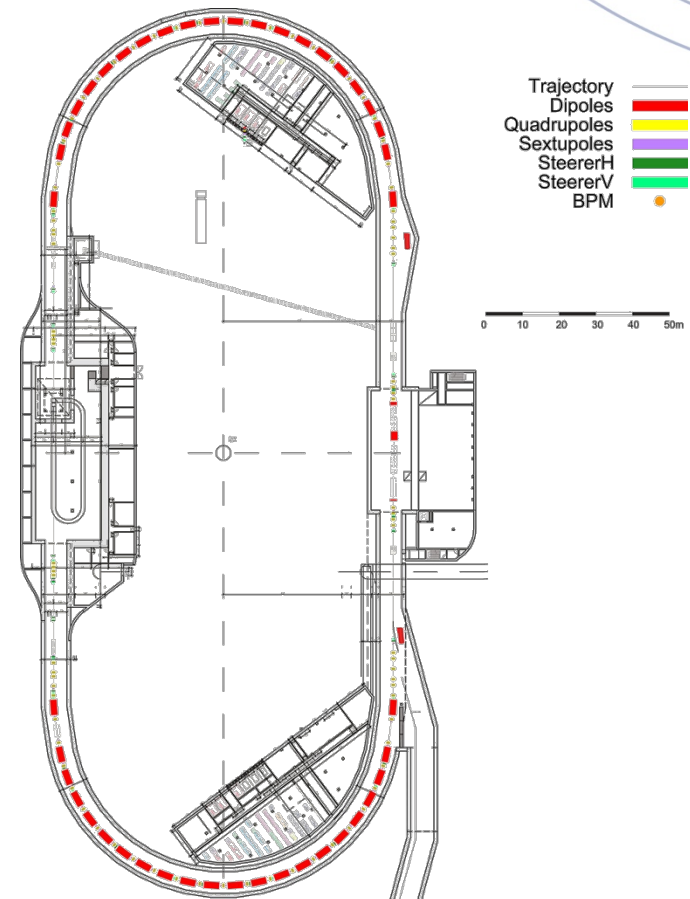




# Accelerator magnet mapper

- 8 sensors @ 76 mm diameter
- Radial layout,  $\pm 0.1$  mm
- Precision mounting holes
- Temperature stabilization  $\sim 0.01\text{C}$ :
  - Thermal vias
  - Cu-core PCB
  - Heater
  - Current regulator
  - Insulation
- On-board electronics:
  - $\mu\text{P}$
  - Temperature sensor
  - Voltage regulator
- USB power & communication
- LabVIEW API




# Heater

- Refractory metals:
  - NiCr , FeCrAl, CuNi
  - Mo, W, Ta, Nb, Cr
- 0.5 mm NiCr plate, 1.7 T
  - // : -0.6  $\mu\text{T}$  (0.4 ppm)
  - $\perp$  : -5  $\mu\text{T}$  (3 ppm)
- Field from heater current:
  - ~4 ADC bits
  - Use AC  $\rightarrow$  no DC offset
  - Coil inductance  $\rightarrow$  roll-off
  - ADC integration  $\rightarrow$  negligible  $>$  ~400 Hz





# Resolution & stability

- Noise:
  - $\pm 4.7 \mu\text{T}$  (100 mT range)
- Drift:
  - Bx, By: 0.07 bits/hour
  - Bz: 0.4 bits/hour
- Conditions:
  - 4 hour preheat
  - 16 hours measurement
  - $80 \text{ mT} \pm 0.5 \mu\text{T}$
  - $35^\circ \pm 0.01^\circ$
  - 3-axis mode



# Zero Gauss Chamber

- Measure initial & final zero-offset; interpolate in time
- Enclose mapper, including drive shaft
- Attenuation goal:  
 $\sim 50 \mu\text{T} \rightarrow < 1 \mu\text{T}$
- Measured:
  - $41.754 \mu\text{T} \rightarrow 0.232 \mu\text{T}$
  - Maximum (orientation)
  - $\sim 6 \text{ mm}$  below sensor



# Conclusions

- Logical evolution of 3-axis Hall magnetometers
- Size, performance, cost → embedded / custom applications, e.g. mappers
- Calibration, UIF → not a “cheap gaussmeter”
- Unsuitable for special conditions (e.g. high precision, low fields, cryogenic temperatures)

